

FIG. 1A

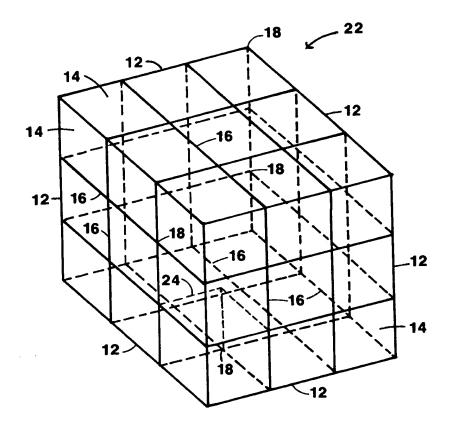
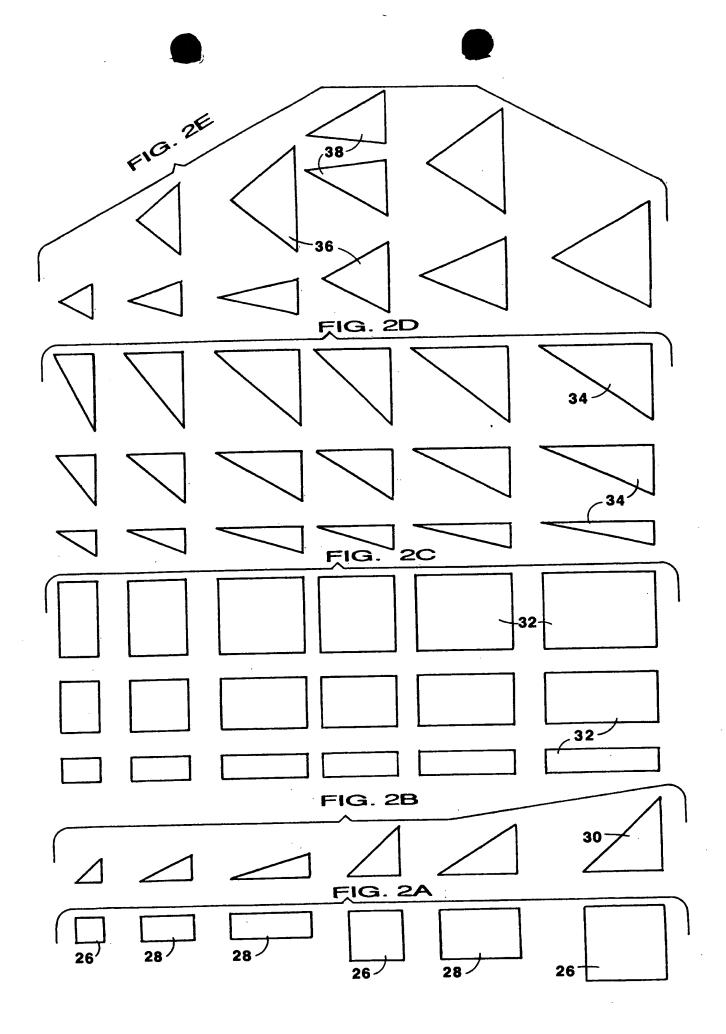
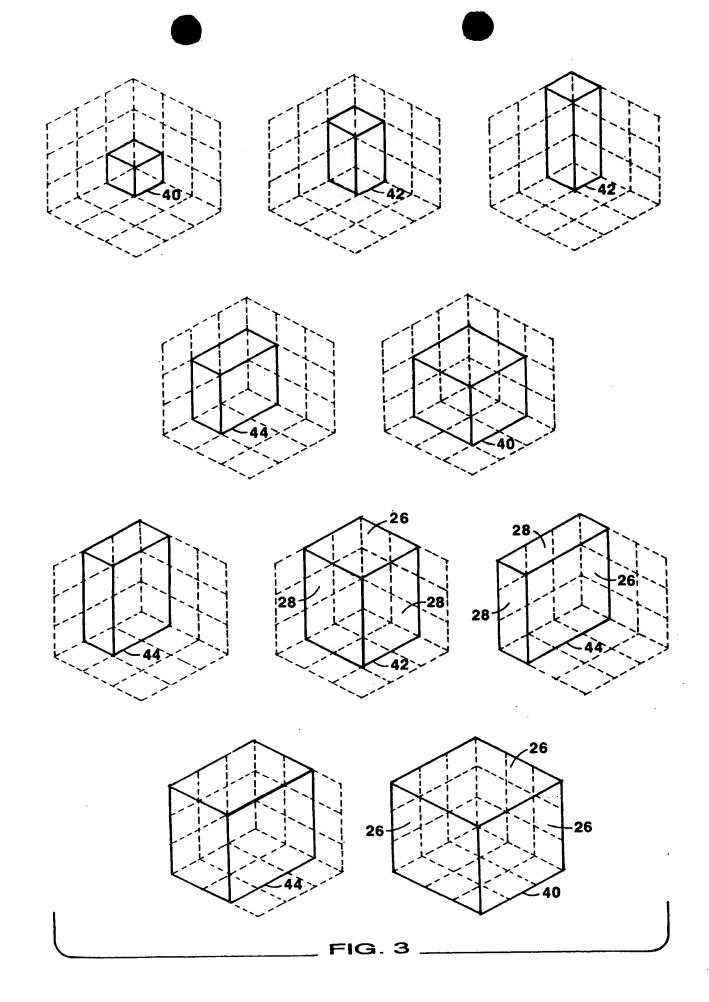
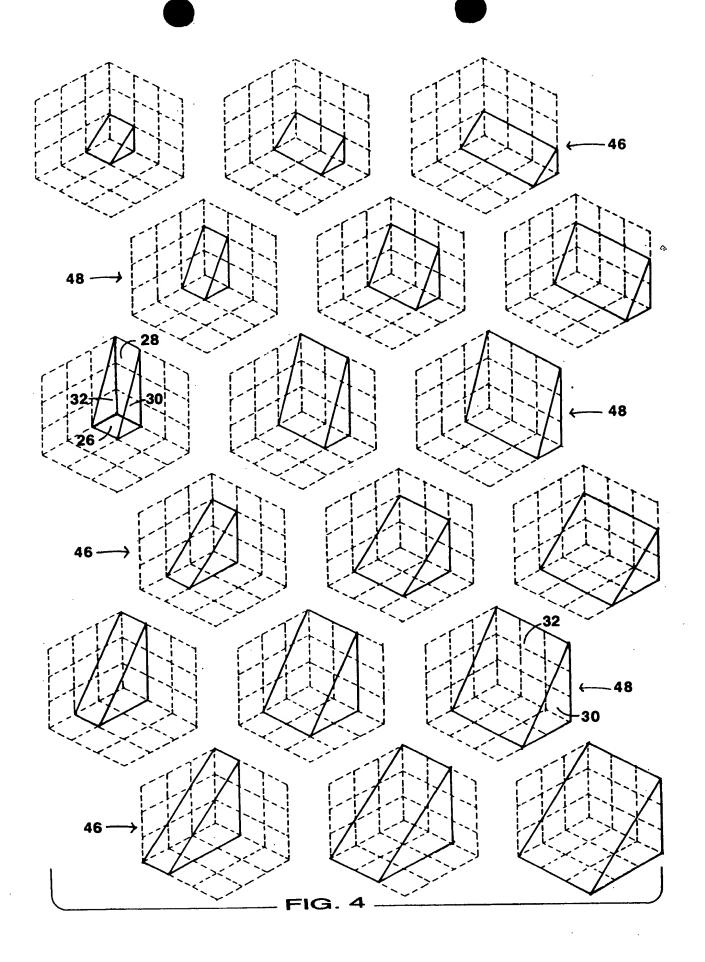
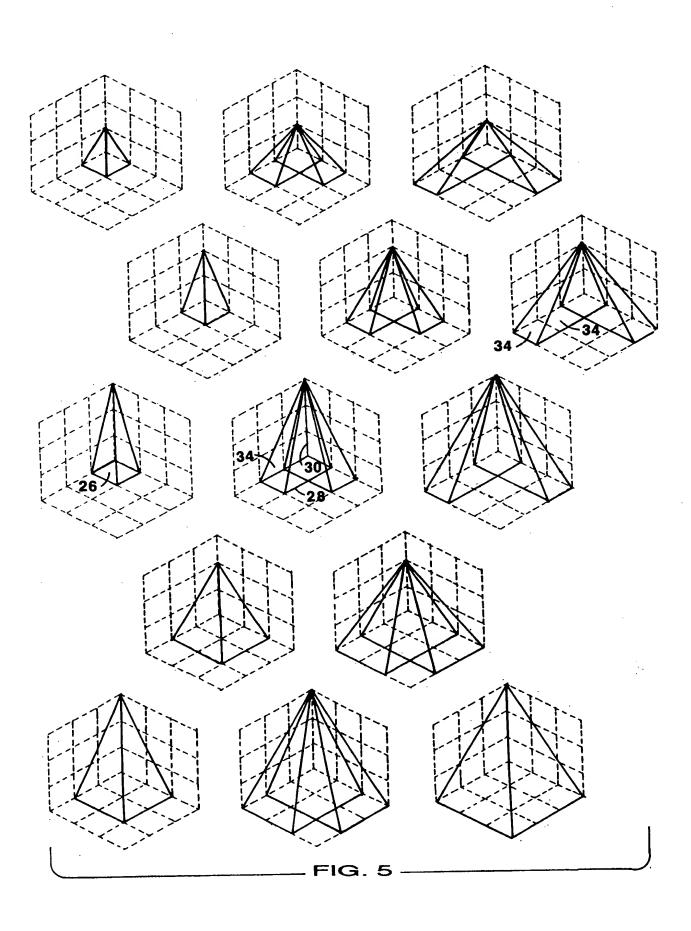



FIG. 1C










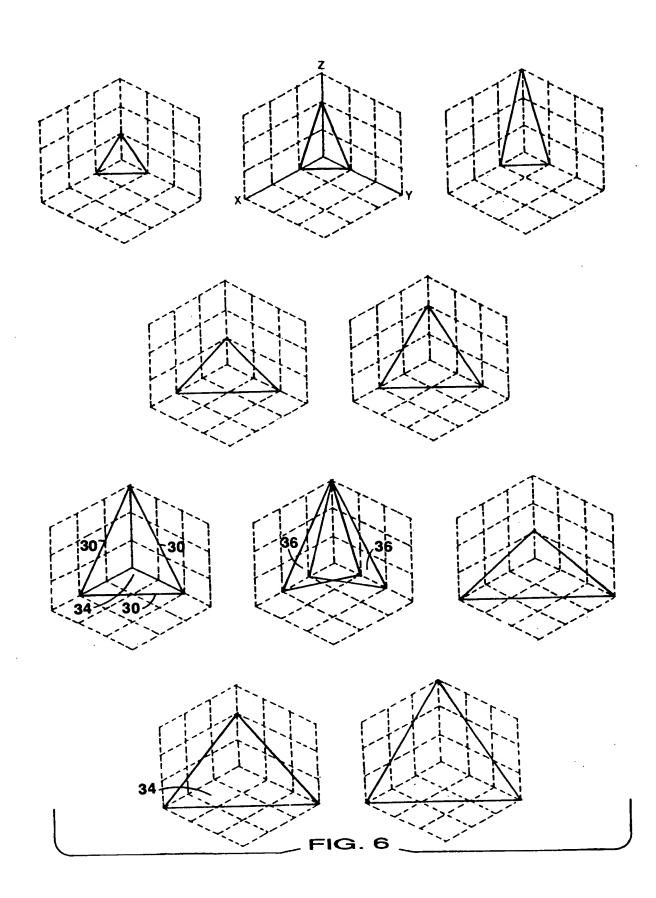

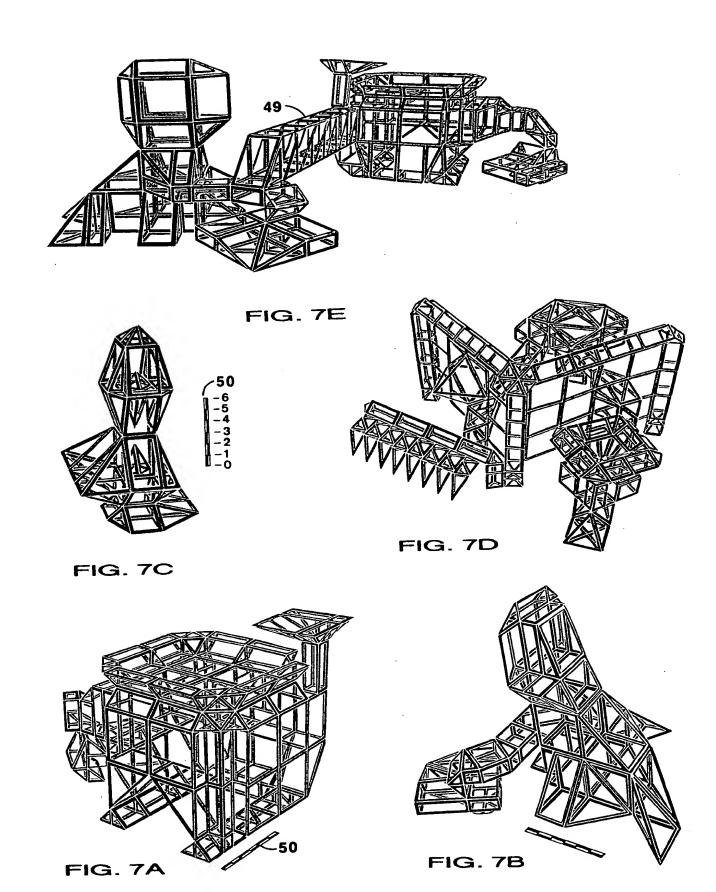

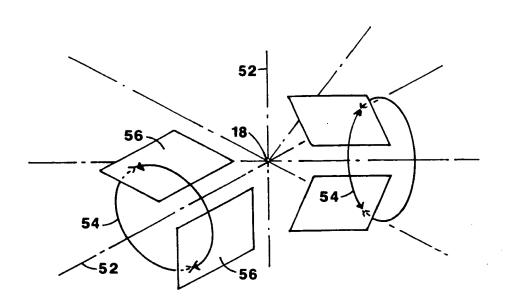


FIG. 8

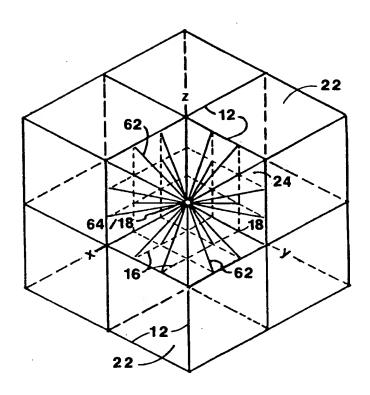


FIG. 9

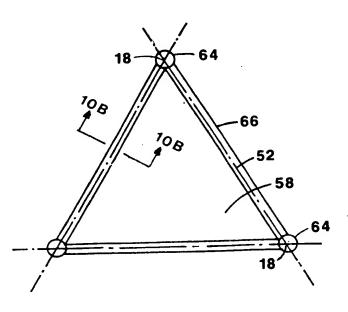


FIG. 10A PRIOR ART



FIG. 10B PRIOR ART




FIG. 10C PRIOR ART




FIG. 10D PREFOR MRT





FIG. 10E

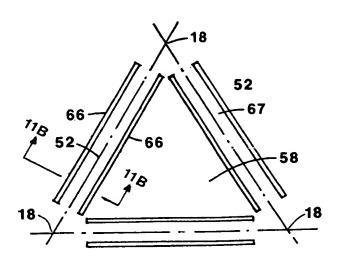

66 67 66

FIG. 11A

FIG. 11B




FIG. 11C




FIG. 11D




FIG. 12

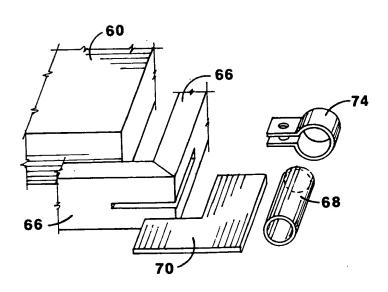


FIG. 13

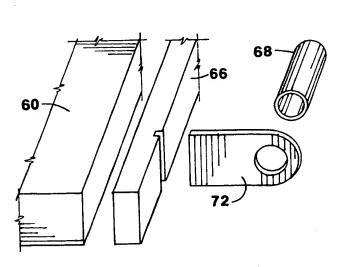


FIG. 15




FIG. 14




FIG. 16

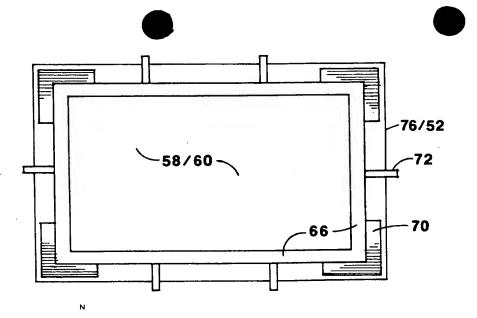
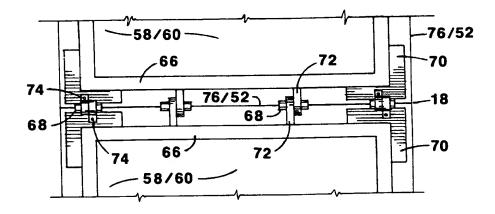


FIG. 17



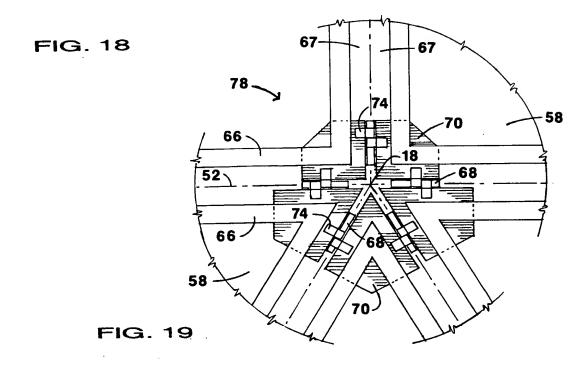
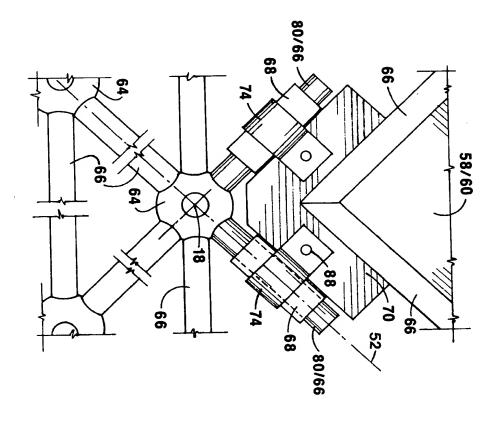
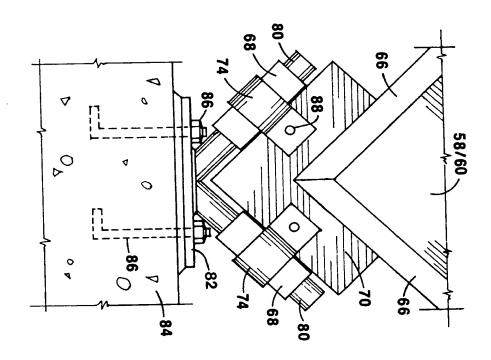
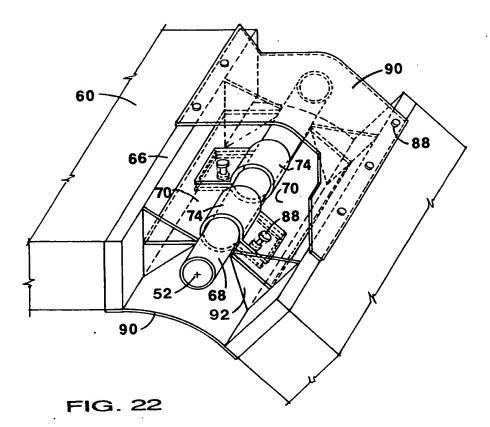


FIG. 20

FIG. 21







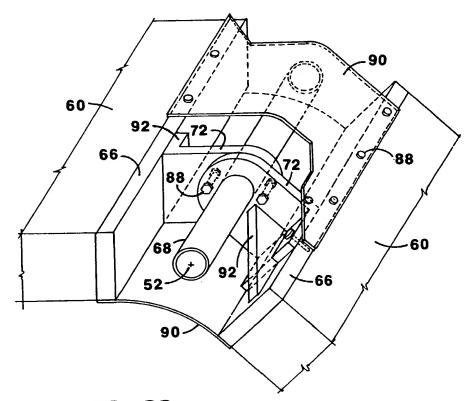


FIG. 23

